


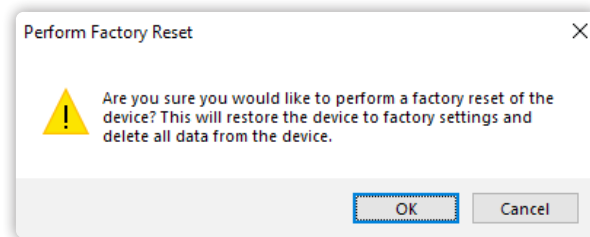
HOW TO: RESET A1s and T3s

 This procedure will erase all data on the device (patient information, BDA number of the oximeter).

Connect the Nox T3s/A1s to a computer and open Noxturnal.



In the Noxturnal software, click on Recording > **Factory Reset** to reset your device.



Click **OK**.
Once the device is restarted, it is completely reset.